



## CGM FAQ

Comparison of CGM Brands and Versions				
	Libre 2	Libre 3	Dexcom G6	Dexcom G7
Placement	Arm	Arm	Abdomen	Arm
Receiver	Reader OR Smart Phone	Smart Phone Only	Reader OR Smart Phone	Reader OR Smart Phone
Need for scanning	Must scan every 8 hours	Automatically uploads every minute	Automatically uploads every 5 minutes	Automatically uploads every 5 minutes
Replacement	14 days	14 days	Sensor - 10 days Transmitter – 3 months	10 days
Warm Up Period	1 hour	1 hour	2 hour	30 mins
Application Video	<a href="https://youtu.be/pHZlr1dprYw">https://youtu.be/pHZlr1dprYw</a>	<a href="https://youtu.be/CRDitmOoIOc">https://youtu.be/CRDitmOoIOc</a>	<a href="https://youtu.be/dBOgdsfeM-A">https://youtu.be/dBOgdsfeM-A</a>	<a href="https://youtu.be/KLbBidcY4IA">https://youtu.be/KLbBidcY4IA</a>
App	Libre View		Dexcom Clarity	

- Tips on placement (wiping with alcohol swap)
  - Ensure you wipe the site of application well in order to get all the oils off the surface which will help the sensor last the full amount of time. Wait for alcohol to wipe fully before placement
  - It may be helpful for patients at home to place a new CGM directly after a shower, fully dry off, then wipe with an alcohol pad. This will decrease the chances the CGM falls off too soon
  - Avoid tight clothing over the sensor
- What to do if the CGM falls off
  - Ask patient if they are comfortable putting another sensor on themselves. If not, schedule them for another education/placement session
  - Have the patient call the manufacturer (Also found of the sensor box):
    - Freestyle Libre: (855)-632-8658
    - Dexcom: (888) 738-3646
- Insurance
  - Medicaid alone or commercial Insurance
    - Send to retail pharmacy
    - May have copay or need of a PA for commercial insurance
  - Medicare or dual Medicare + Medicaid
    - Patient must have Ha1c > 7.5 and on insulin therapy
    - Must go through DME process

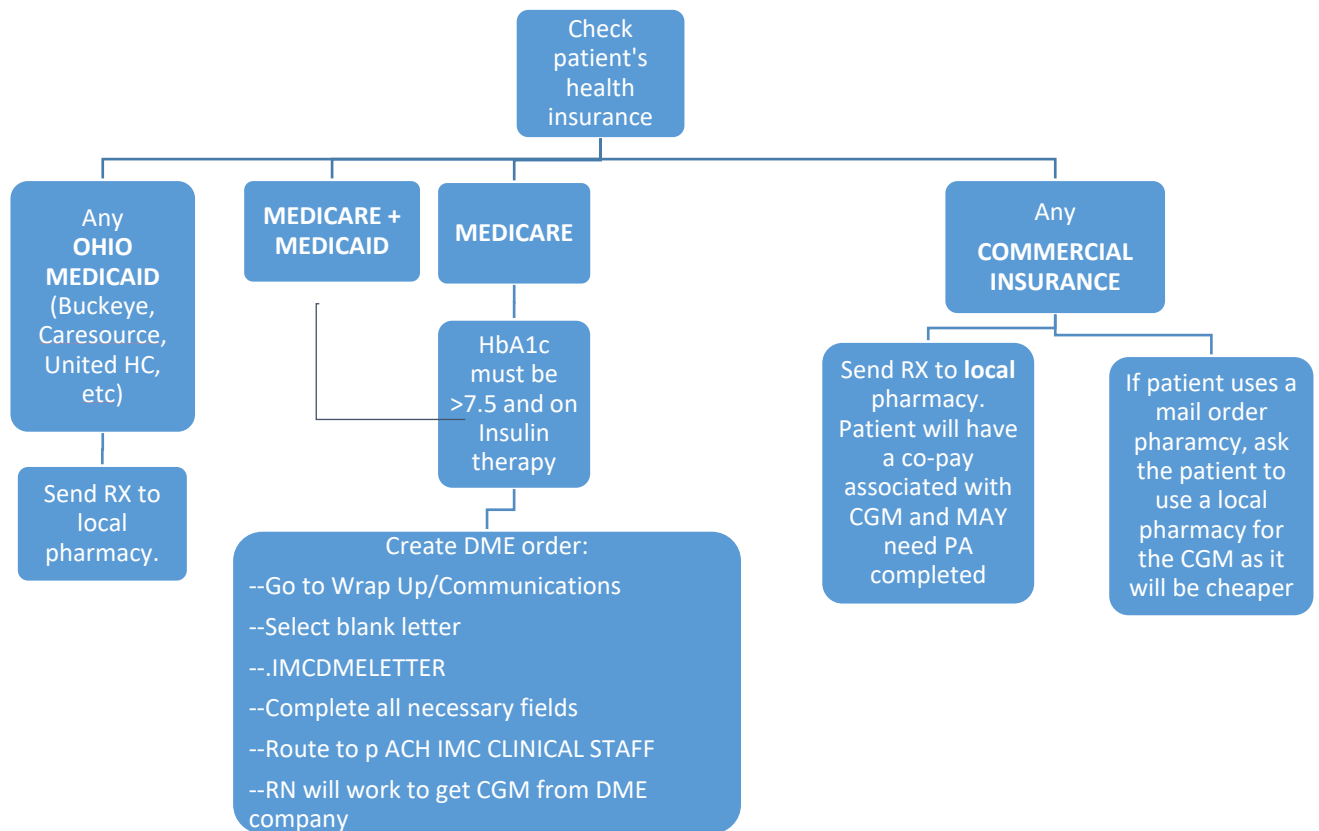

- Dexcom Clarity and Libre View
  - Decom Clarity (Smart phone)
    - Tap Profile > Authorize Sharing and follow the instructions
      - Smart phone will give a code for the provider into input into Dexcom Clarity website for report generation
  - LibreView App (Smart phone)
    - Menu > Connected Apps > LibreView > Connect to a Practice > Enter Practice ID
    - Practice ID: 330-375-3315
      - Make sure you include the hyphens when inputting the code
  - Libre Reader
    - Reader must be brought to the visit for report generation
      - Log into the LibreView website
      - Connect the reader to your computer (port is on the side of the reader)
      - Click on “Press to Begin Upload”. Do not disconnect the reader while the upload is in progress. The glucose history screen will open up.
- 2 visits
  - Schedule education/placement
    - 2 weeks post sending to retail pharmacy (Medicaid)
    - 4 weeks after starting the DME process (Medicare)
  - Schedule reading/interpretation 2 weeks after education/placement

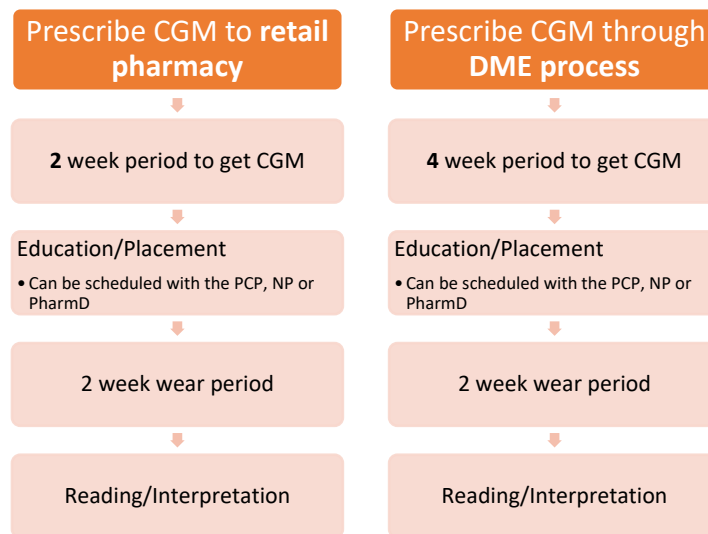

- Lost sensor
  - A new sensor prescription can be sent
  - Depending on the insurance, the patient may be able to get 1 replacement per year